

Version 2.1 Software

Addendum to the IQ plus 510 and 710 Installation Manuals

Version 2.1 software for the IQ plus 510 and 710 indicator provides the following capabilities:

- SMPRAT parameter added to the CONFIG menu to allow selection of A/D sample rate in samples per second (see Figure 1). Lower sample rate values provide greater signal noise immunity.
- YYMMDD date format added to the DATEFMT parameter on the PROGRM menus (see Figure 2).

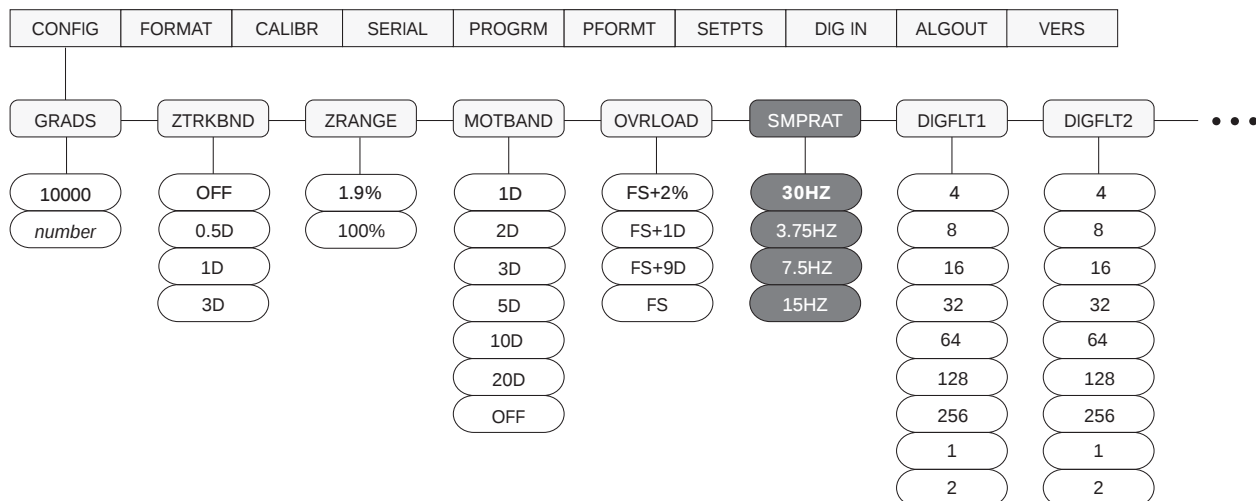


Figure 1. Partial IQ plus 710 Version 2.1 CONFIG Menu, showing location of SMPRAT Parameter

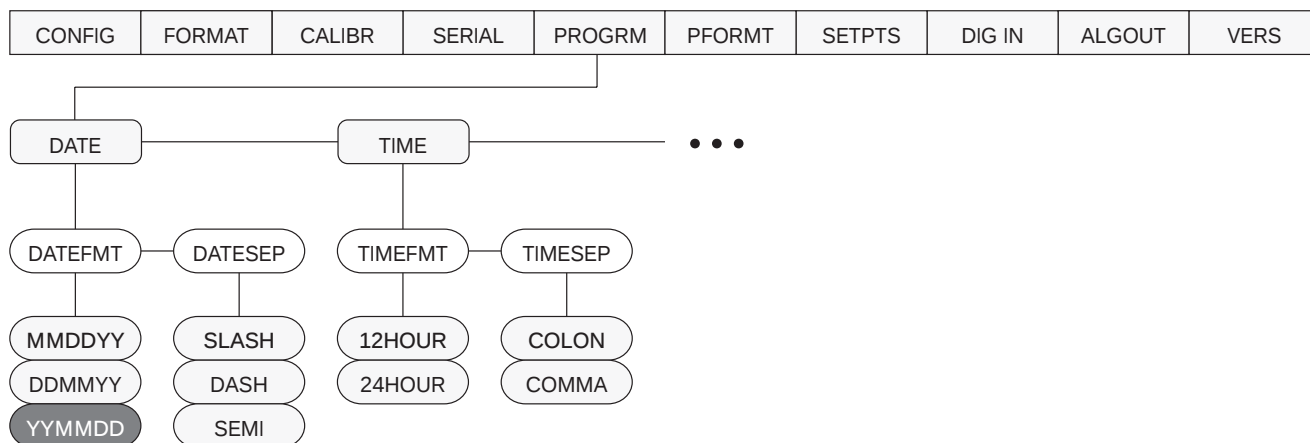


Figure 2. Partial IQ plus 710 Version 2.1 PROGRM Menu, Showing Changed DATEFMT Parameter