



Consumer and
Corporate Affairs Canada

Legal Metrology

Consommation
et Corporations Canada

Métrieologie légale

APPROVAL No. - N° D'APPROBATION

S.WA-3126

MAR 7 1983

NOTICE OF APPROVAL

AVIS D'APPROBATION

THIS NOTICE OF APPROVAL SUPERSEDES
S.WA-T242 DATED October 14, 1982.

LE PRESENT AVIS REMPLACE L'AVIS
S.WA-T242 EN DATE DU 14 octobre 1982.

Company: Toledo Scale Division of
Reliance Electric Limited
5220 Creekbank Road
Mississauga, Ontario

Société: Toledo Scale Division of
Reliance Electric Limited
5220 Creekbank Road
Mississauga, Ontario

Manufacturer: Toledo Scale Division of
Reliance Electric Limited
2462 Howard Avenue
Windsor, Ontario

Fabricant: Toledo Scale Division of
Reliance Electric Ltd.,
2462 Howard Avenue
Windsor, Ontario

Type of Device: Electronic low profile
dormant scale.

Appareil: Pont-basculé électronique
surbaissé.

<u>MODEL NUMBER</u> <u>No. de modèle</u>	<u>CAPACITY</u> <u>Capacité</u>
2155	36" x 36" 48" x 48" 60" x 60"

<u>PLATFORM SIZE (in.)</u> <u>Dimension du tablier (po.)</u>
1000 lb. OR/ou 500 kg. 2000 lb. OR/ou 1000 kg. 5000 lb. OR/ou 2500 kg.

Suffix EG with model number denotes the
stainless steel version.

Les modèles dont le numéro se termine
par EG sont en acier inoxydable.


Accessories: Compatible accessories that
meet the requirements and perform in
accordance with the Weights and Measures
Act, Regulations and Specifications may
be used.

Accessoires: Peuvent être utilisés tous
les accessoires compatibles qui
satisfont aux exigences de la Loi, du
règlement et des prescriptions
ministérielles régissant les poids et
mesures.

Description: This device is a fully
electronic low profile dormant scale with
a bending beam type load cell at each
corner. A retainer with a steel ball is
fastened to the sub-frame under each load
cell. The steel ball fits into a socket
on the load cell. The junction box is
located within the platform frame.

Description: Il s'agit d'un pont-
basculé surbaissé entièrement électro-
nique comportant à chacun des coins un
dynamomètre de cisaillement. Un dispo-
sitif de retenue à bille d'acier est
fixé à la sous-structure sous chaque
dynamomètre. Les billes d'acier
s'insèrent dans une douille installée
sur les dynamomètres. La boîte de
jonction est située à l'intérieur de la
structure formant le tablier.

.../2

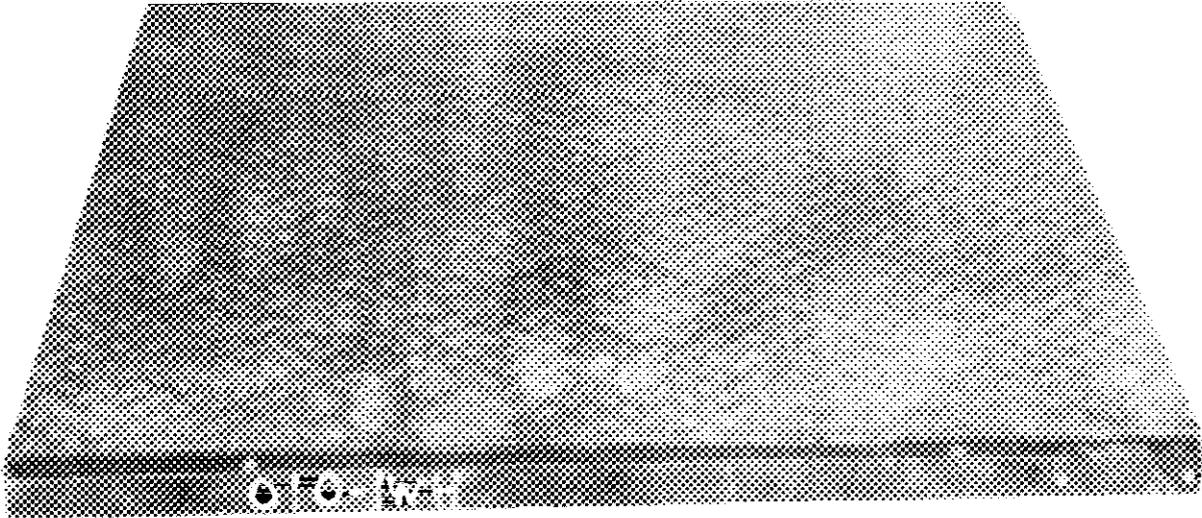

Description: Continued

The unit may have up to four(4) steel ramps giving access to the platform in all directions. The scale may be installed in a shallow pit without ramps.

Conditions of Approval: Approval is granted under the Weights and Measures Act, S.C. 1970-71-72, chapter 36, and the Weights and Measures Regulations C.R.C.c., 1605 for use in Canada under the general conditions of the said Regulations, and under any special conditions listed above.

Reference No.: G6922-T170-10

Chief
Legal Metrology Laboratories

Description: Suite

La bascule peut comporter jusqu'à quatre (4) rampes en acier permettant d'y accéder de tous les sens. Elle peut également être installée dans une fosse peu profonde sans rampes d'accès.

Condition d'approbation: L'approbation est accordée conformément à la Loi sur les poids et mesures S.R.C. 1970-71-72, chapitre 36, et au règlement d'application C.R.C.c., 1605. L'emploi est autorisé au Canada sous réserve des conditions générales dudit règlement, et de toutes les conditions particulières formulées dans le présent avis.

No. de référence: G6922-T170-10

Chef
Laboratoires de la Métrologie légale


W.R. Virtue

MAR 7 1983